

## VACUETTE® BLOOD COLLECTION TUBES

### ITEM N° 454410



#### Characterisation

VACUETTE® TUBE 4 ml K2E K2EDTA 13x75 lavender cap-black ring, transparent label, non-ridged

#### Intended Use

VACUETTE® Blood Collection Tubes, Holders and Needles are used together as a system for the collection of venous blood. VACUETTE® tubes are used to collect, transport, store and process blood for testing serum, plasma or whole blood in the clinical laboratory and are for professional use.

#### Description

Dimension	13x75 mm
Capacity	4 ml
Cap colour	lavender
Ring colour	black

#### Materials

PET Polyethylene terephthalate	Tube
Transparent	Label
PE Polyethylene	Cap
PP Polypropylene	Ring
Bromobutyl rubber, non-latex	Rubber stopper
Separator	/ none used
Latex	/ none used
Phthalates	/ none used

#### Additive

K<sub>2</sub> EDTA

#### Manufacturer

Legal Manufacturer:  
Greiner Bio-One GmbH  
Bad Haller Str. 32  
A-4550 Kremsmünster

**Note:** Printed copies will not systematically be updated. Valid at the date of issue. Information is subject to change.

## Sterilisation

Sterile interior: SAL  $10^{-6}$  (SAL = Sterility Assurance Level)  
Standard: ISO 11137

## Directive

IVDD 98/79/EC "Directive 98/79/EC of the European Parliament and council of 27th of October 1998 on in vitro diagnostic medical devices" Classification: Other device (all devices except Annex II and self-testing devices)

## Product Storage

Store tubes at 4–25°C (40–77°F).  
NOTE: Avoid exposure to direct sunlight. Exceeding the maximum recommended storage temperature may lead to impairment of the tube quality (i.e. vacuum loss, drying out of liquid additives, colouring, etc.)

## Shelf Life

16 months

## Disposal










1. The general hygiene guidelines and legal regulations for the proper disposal of infectious material should be considered and followed.
2. Disposable gloves prevent the risk of infection.
3. Contaminated or filled blood collection tubes must be disposed of in suitable biohazard disposal containers, which can then be autoclaved and incinerated afterwards.
4. Disposal should take place in an appropriate incineration facility or through autoclaving (steam sterilisation).

## Packaging

24 racks of 50 pcs., 1200 pcs. in total




## Label information

According to ISO 15223-1, for use in the labelling of medical devices.

Symbol	Description	Symbol	Description
	Manufacturer		Temperature limit
	Use-by date		Do not re-use
	Batch code		Consult instructions for use
	Catalogue number		In vitro diagnostic medical device
	Sterilized using irradiation		

# PRODUCT SPECIFICATION

## Labelling

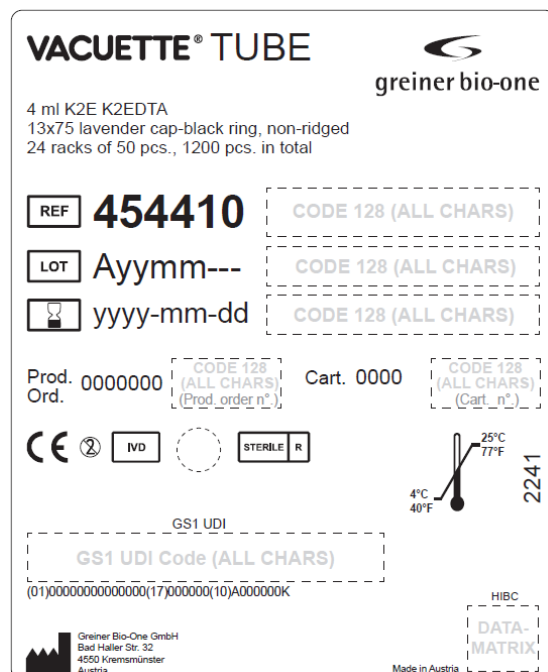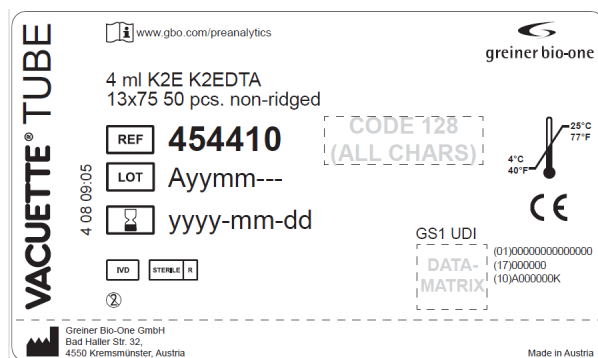

**Note:** Printed copies will not systematically be updated. Valid at the date of issue. Information is subject to change.